

REFERENCE

UNITED STATES  
DEPARTMENT OF  
COMMERCE  
PUBLICATION



# NBS TECHNICAL NOTE 776

## A New Method for Generating Waterdrops of Specified Mass

U.S.  
DEPARTMENT  
OF  
COMMERCE

National

QC — U  
OO of  
Is

5753

776

173

## NATIONAL BUREAU OF STANDARDS

The National Bureau of Standards<sup>1</sup> was established by an act of Congress March 3, 1901. The Bureau's overall goal is to strengthen and advance the Nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research and provides: (1) a basis for the Nation's physical measurement system, (2) scientific and technological services for industry and government, (3) a technical basis for equity in trade, and (4) technical services to promote public safety. The Bureau consists of the Institute for Basic Standards, the Institute for Materials Research, the Institute for Applied Technology, the Center for Computer Sciences and Technology, and the Office for Information Programs.

**THE INSTITUTE FOR BASIC STANDARDS** provides the central basis within the United States of a complete and consistent system of physical measurement; coordinates that system with measurement systems of other nations; and furnishes essential services leading to accurate and uniform physical measurements throughout the Nation's scientific community, industry, and commerce. The Institute consists of a Center for Radiation Research, an Office of Measurement Services and the following divisions:

Applied Mathematics — Electricity — Mechanics — Heat — Optical Physics —  
Linac Radiation<sup>2</sup> — Nuclear Radiation<sup>2</sup> — Applied Radiation<sup>2</sup> — Quantum  
Electronics<sup>3</sup> — Electromagnetics<sup>3</sup> — Time and Frequency<sup>3</sup> — Laboratory  
Astrophysics<sup>3</sup> — Cryogenics<sup>3</sup>.

**THE INSTITUTE FOR MATERIALS RESEARCH** conducts materials research leading to improved methods of measurement, standards, and data on the properties of well-characterized materials needed by industry, commerce, educational institutions, and Government; provides advisory and research services to other Government agencies; and develops, produces, and distributes standard reference materials. The Institute consists of the Office of Standard Reference Materials and the following divisions:

Analytical Chemistry—Polymers—Metallurgy—Inorganic Materials—Reactor  
Radiation—Physical Chemistry.

**THE INSTITUTE FOR APPLIED TECHNOLOGY** provides technical services to promote the use of available technology and to facilitate technological innovation in industry and Government; cooperates with public and private organizations leading to the development of technological standards (including mandatory safety standards), codes and methods of test; and provides technical advice and services to Government agencies upon request. The Institute also monitors NBS engineering standards activities and provides liaison between NBS and national and international engineering standards bodies. The Institute consists of a Center for Building Technology and the following divisions and offices:

Engineering and Product Standards—Weights and Measures—Invention and  
Innovation—Product Evaluation Technology—Electronic Technology—Technical  
Analysis—Measurement Engineering—Building Standards and Code Services<sup>4</sup>—Housing Technology<sup>4</sup>—Federal Building Technology<sup>4</sup>—Structures, Materials and Life Safety<sup>4</sup>—Building Environment<sup>4</sup>—Technical Evaluation and  
Application<sup>4</sup>—Fire Technology.

**THE INSTITUTE FOR COMPUTER SCIENCES AND TECHNOLOGY** conducts research and provides technical services designed to aid Government agencies in improving cost effectiveness in the conduct of their programs through the selection, acquisition, and effective utilization of automatic data processing equipment; and serves as the principal focus within the executive branch for the development of Federal standards for automatic data processing equipment, techniques, and computer languages. The Center consists of the following offices and divisions:

Information Processing Standards—Computer Information—Computer Services  
—Systems Development—Information Processing Technology.

**THE OFFICE FOR INFORMATION PROGRAMS** promotes optimum dissemination and accessibility of scientific information generated within NBS and other agencies of the Federal Government; promotes the development of the National Standard Reference Data System and a system of information analysis centers dealing with the broader aspects of the National Measurement System; provides appropriate services to ensure that the NBS staff has optimum accessibility to the scientific information of the world, and directs the public information activities of the Bureau. The Office consists of the following organizational units:

Office of Standard Reference Data—Office of Technical Information and  
Publications—Library—Office of International Relations.

<sup>1</sup> Headquarters and Laboratories at Gaithersburg, Maryland, unless otherwise noted; mailing address Washington, D.C. 20234.

<sup>2</sup> Part of the Center for Radiation Research.

<sup>3</sup> Located at Boulder, Colorado 80302.

<sup>4</sup> Part of the Center for Building Technology.

100  
5753  
776  
973

at acc - Ref

# A New Method for Generating Waterdrops of Specified Mass

---

James E. Potzick

Mechanics Division  
Institute for Basic Standards  
National Bureau of Standards  
Washington, D.C. 20234

U.S.

*Technical note, no. 776*  
Sponsored by  
Fluid Dynamics Program  
Office of Naval Research  
U.S. Department of the Navy  
Washington, D.C. 20360

NBS Technical Notes are designed to supplement the Bureau's regular publications program. They provide a means for making available scientific data that are of transient or limited interest. Technical Notes may be listed or referred to in the open literature.




---

U.S. DEPARTMENT OF COMMERCE, Frederick B. Dent, Secretary  
NATIONAL BUREAU OF STANDARDS, Richard W. Roberts, Director

Issued May 1973

**National Bureau of Standards Technical Note 776**

**Nat. Bur. Stand. (U.S.), Tech. Note 776, 12 pages (May 1973)**

**CODEN: NBTNAE**



# A New Method for Generating Waterdrops of Specified Mass\*

James E. Potzick

A waterdrop generator has been constructed, based on the mechanical resonance of a vibrating waterdrop, which can generate drops of 1.5 to 37 mg with standard deviations in the range of 0.1 percent to 10 percent of drop mass. Drop mass over this range and drop interval are remotely controlled.

Key words: Drop generator; liquid drop; waterdrop.

## 1. Introduction

Water is one of the most useful and abundant substances on our planet and is the subject of a great deal of research. Much has been written concerning the behavior of waterdrops [1-5]\*\*, and in preparation for a study continuing this research, a new type of waterdrop generator was developed using what is believed to be a hitherto unexploited operating principle.

Most waterdrop generators seem to fall into three categories. The simplest type allows water to drip from the end of a capillary tube [1,6]. The size of the drop depends primarily on the outer diameter of the tube. This type of generator is characterized by simplicity, excellent repeatability of drop size, and lack of flexibility.

A more sophisticated type of waterdrop generator is based on a phenomenon described by Rayleigh [7] nearly a century ago in which a jet of water issuing from a capillary tube is broken into uniform drops by vibrating the capillary at the proper frequency [8,10-14]. This produces a continuous stream of drops whose separation is on the order of a drop diameter. The size of the drops depends primarily on the flow rate and the diameter of the tube, and, over a narrow range, on the frequency of vibration.

In addition, there are other types of waterdrop generator which use some means such as an air blast [15,16], rapid acceleration of the capillary tube, or electrostatic force [9] to detach a drop of given size from the end of a capillary tube.

While each of these waterdrop generators has its merits, a more flexible generator is needed for the impending study, with the following properties: drop size and interval between drops must be remotely controlled so the generator can be located where access is difficult; drop size must be continuously adjustable; uncharged or arbitrarily charged drops must be available for studies of electrostatic effects; the time interval between drops must be variable from several seconds to infinity, i.e., single drops must be available on demand.

A waterdrop generator has been developed which meets all of these requirements to a reasonable degree. In this generator water is allowed to drip from a nozzle as in the first type of generator described above, but to generate drops of arbitrary size the nozzle is vibrated vertically at a low frequency while the drop is slowly growing at the end of the nozzle. When the resonant frequency of the drop approaches the vibrating frequency, the drop falls. For a given nozzle the mass of the drop is determined by the frequency of vibration, and the present apparatus can generate drops from 1.5 mg to 37 mg with a standard deviation from 10 percent to 0.1 percent of drop mass, with one nozzle. Other mass ranges can be covered with different size nozzles. A remotely actuated solenoid valve can be used to stop the water flow between drops. One might object that the drop continues to vibrate while it is falling, but this is true of drops generated by other methods as well [3,7,17], and is an important consideration in the study of water drop impacts. The vibrating pendant waterdrop may be useful in other areas of water research, such as in studies of surface properties or viscosity measurements. And of course other liquids besides water can be used.

\*This research is part of a study sponsored by the Fluid Dynamics Program, Office of Naval Research, Department of the Navy, Arlington, Virginia 22217.

\*\*Figures in brackets indicate literature references at the end of this paper.

## 2. Principle of Operation

Figure 1 shows a waterdrop hanging from a nozzle. If the nozzle vibrates vertically with a small amplitude, the vibrating drop will assume the shapes shown in the sketch, figure 2; one might say the drop appears alternately squeezed and stretched. At a sufficiently large amplitude the neck of the drop in the "stretch" position will go to zero diameter and the drop will fall. This could be called an infinite amplitude state.

The resonant frequency of the pendant drop is a monotonic function of its mass. In operation the amplitude of the nozzle vibration is chosen and kept constant so that, as the drop mass grows slowly, its amplitude grows and reaches the infinite amplitude state as its resonant frequency approaches the operating frequency. In this way the mass of the falling drop is chosen by selecting the frequency of vibration. Figures 3 and 4 show water drops vibrating near their resonant frequencies at 40 and 90 Hz, respectively.

Note that this method of generating waterdrops is different from Rayleigh's method, since he writes of periodic disturbances propagating down a falling stream of water, breaking it into drops, and there is no stream here, the drops forming individually at arbitrarily long intervals. At zero frequency, of course, the vibrating waterdrop generator is identical with the stationary capillary tube type described above. Mason, et al. [13], write of their vibrating hypodermic needle apparatus that the needle may undergo several cycles at low flow rates before a drop is dispatched, but they were primarily interested in Rayleigh's method, and their frequency was fixed.

No analytical treatment of the vibrating drop is attempted here.

## 3. Description

The apparatus is shown in figures 5 and 6. A small moving coil vibrator is connected to the stainless steel armature and nozzle by a flexible link made from a piece of plastic tubing. The armature slides vertically in a brass bearing and is lubricated with a thin film of light oil to reduce distortion in the sinusoidal motion due to Coulomb friction. An air bearing could be used here to advantage. There is a small permanent magnet inside the armature and a wire coil wound around the brass bearing so that the motion of the armature can be monitored by observing the voltage across the coil.

Interchangeable nozzles are screwed into the bottom of the armature and water is supplied from the reservoir through a short length of very small rubber tubing of the kind used to supply ink to recorder pens. This tubing slips over a piece of hypodermic needle which is press-fitted into the armature. Water is supplied by gravity feed from a reservoir located above the apparatus through a flow regulating needle valve and a remotely controlled solenoid shutoff valve.

The nozzle is made of stainless steel and has a flat bottom of 2.3 mm diameter, with a sharp edge. The hole is 0.34 mm diameter (No. 80 drill), and the conical side of the nozzle is polished. A hemispherical tip was tried for the nozzle, but the extent of the surface which the water was to wet was then not well-defined; about twice the vibration amplitude was needed to generate drops, and only a small range of drop sizes could be accommodated. After the drop has left the nozzle it falls between a photocell and lamp, generating an electrical pulse which signals its arrival.

A block diagram of the system is shown in figure 7. A digitally tuned oscillator is used to facilitate accurate and repeatable frequency setting. This oscillator drives the vibrator through an amplitude regulator and power amplifier. The low voltage signal from the monitor coil is amplified and used to monitor the amplitude and waveshape of the armature motion. A differential amplifier must be used here to avoid pickup from the vibrator drive current in the long cable to the waterdrop generator.

There is some small dependence of the waterdrop mass on vibration amplitude (see below) and so an amplitude regulator, based on a design described previously [18], is used to hold the monitor coil voltage to a constant amplitude. When the vibrator is turned on, for instance, the armature motion warms the oil, reducing its viscosity. Without the regulator the vibration amplitude would increase. The regulator cannot be used at frequencies below



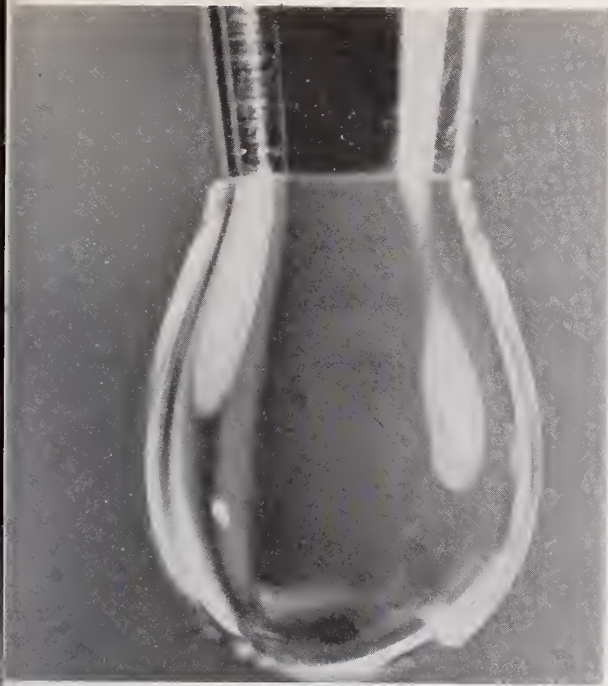


Figure 1. Stationary waterdrop hanging from nozzle.

Figure 2. Sketch of vibrating waterdrop in its simplest mode of vibration near its resonant frequency.

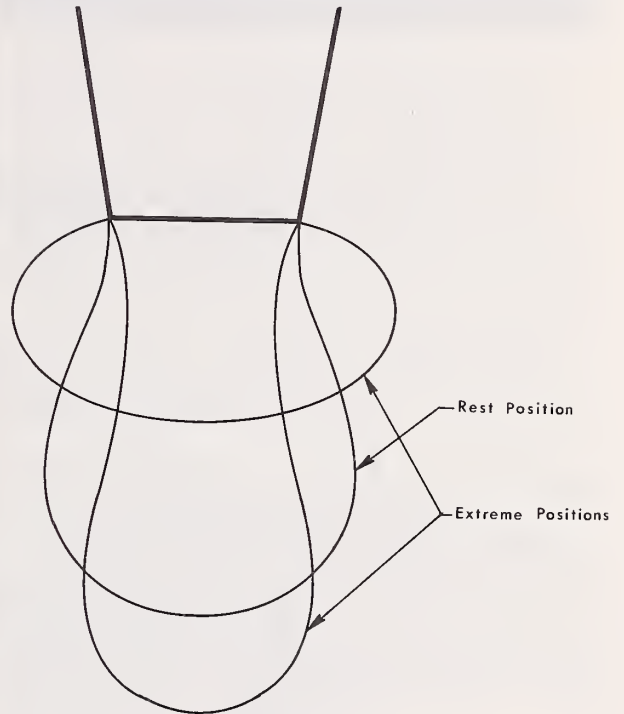


Figure 3. Vibrating waterdrop at 40 Hz shortly before detachment - incipient 6.8 mg drop.

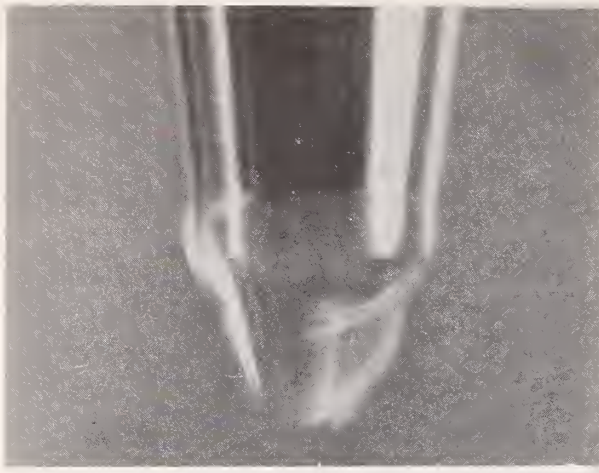


Figure 4. Vibrating waterdrop at 90 Hz shortly before detachment - incipient 1.5 mg drop.

Figure 5. Photograph of waterdrop generator. Vibrator is not seen in this view.


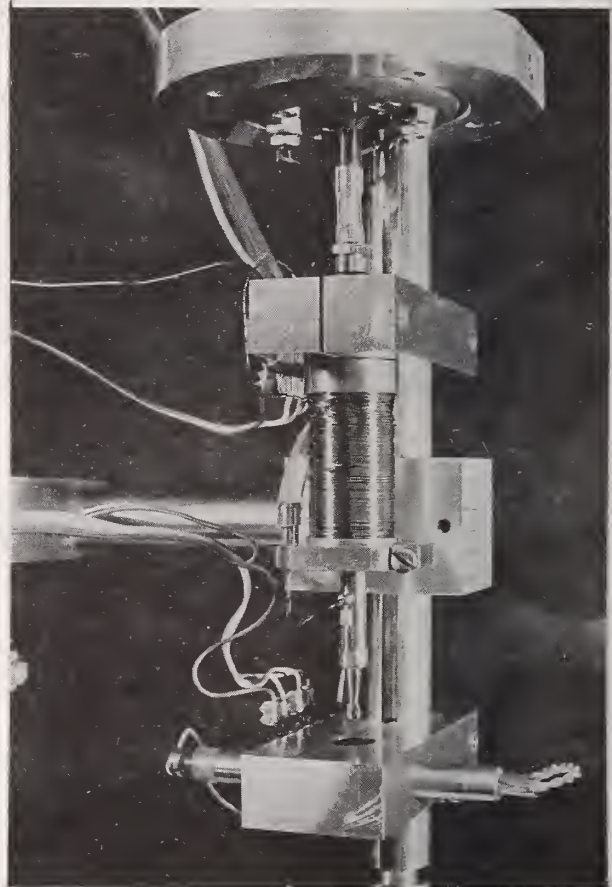


Figure 6. Mechanical construction of waterdrop generator.

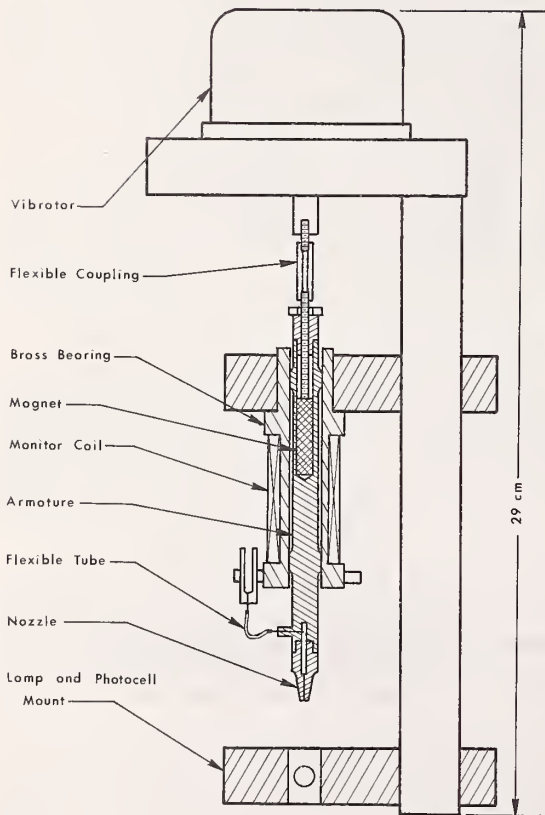

about 10 Hz.

The apparatus can generate waterdrops continuously (at intervals of several seconds) by leaving the vibrator on and the solenoid valve open. A single drop mode, or "demand mode," can be used, however, in which a single drop is generated when the "Initiate" button is pushed. This sets the flip-flop in figure 7, opening the solenoid valve and turning on the vibrator. When the drop falls the photocell generates a pulse which resets the flip-flop, closing the valve and turning off the vibrator. This pulse is also useful for announcing the approach of the waterdrop to downstream equipment.

#### 4. Performance

Ordinary distilled water was used during calibration of the waterdrop generator. The flow rate was adjusted with the needle valve to about 37 mg/min and seemed to be independent of the waterdrop mass. The only apparent requirement on the flow rate is that it be low enough so that each drop grows slowly compared to the transient motions that occur at detachment and forming of a new drop.

It would seem that at each frequency there should be an optimum amplitude of vibration at which drops form reliably and uniformly. Obviously at zero amplitude one obtains the largest drops regardless of frequency; on the other hand, if the amplitude is too large, drops will be flung off the nozzle before they have a chance to resonate. Figure 8 shows two curves of drop mass as a function of amplitude, the results of a little experiment in which drops were formed over a range of vibration amplitudes at each of two fixed frequencies. The curve for each frequency is discontinuous, and where the segments overlap the probability that a drop will fall on the lower segment increases with increasing amplitude. In normal operation the amplitude is chosen so that the lowest segment is used. Note there is some small slope to the curve here so that the mass depends to some extent on amplitude as well as frequency. In the present case the amplitude was chosen rather arbitrarily and is shown in figure 9. If the optimum amplitudes were known, a frequency response network could be inserted in the vibrator control circuit to insure that the optimum amplitude is used at each frequency. This would probably improve the waterdrop generator's performance.

In calibrating the generator 200 waterdrops were generated and weighed over a period of eight days at ten frequencies from 0 to 90 Hz. Each drop was caught in a small aluminum pan, covered with a small inverted aluminum cup to discourage evaporation, and weighed on an analytical balance to a resolution of 0.1 mg. The zero offset of the balance was checked and readjusted after every 3 to 5 drops and this drift error was assumed to be distributed linearly over these drops, whose weights were correspondingly adjusted. The apparatus was generating drops continuously, so that only every fifth drop or so was weighed. When the demand mode is used it is recommended that several drops be generated and discarded before one is used so that neither too much nor too little water is on the nozzle as the drop begins to form. Then, of course, the continuous mode calibration will apply.

In generating waterdrops by various methods a small droplet called a satellite is sometimes formed with the drop [7,10,11,19]. During calibration of the waterdrop generator satellites were seen in the weighing pan about 15 percent of the time (if a satellite falls on top of the drop it would not be seen). In each case the mass of the satellite was estimated to be less than 1 percent of the mass of the drop.

The lateral scatter of the falling drops appears to be fairly low, since they nearly all fell into the center of the weighing pan, which was placed in the same position each time. The larger drops have less lateral scatter than the smaller ones.

The results of the waterdrop generator calibration are presented in table 1, where the daily average masses  $m_i$  (where  $i$  refers to day 1 through 5) are given for drops at ten frequencies on five different days. All of the drops which were collected and weighed are included. The pooled average mass  $m_p$  at each frequency is the average of the five  $m_i$ 's. The pooled corrected standard deviations were calculated from

$$\sigma_{pc} = \sqrt{\sum_{i=1}^5 \left( \frac{\sigma_i^2}{5} \right) - \sigma_w^2}$$

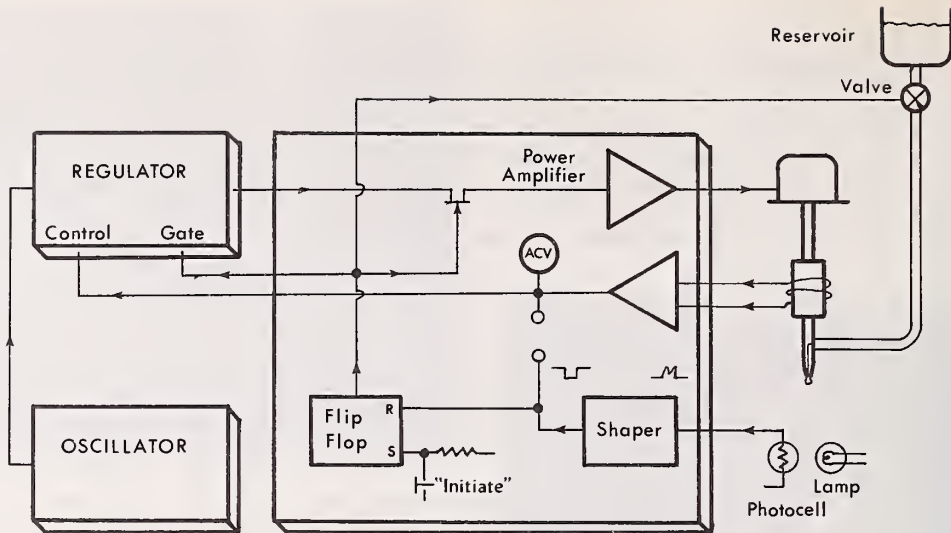


Figure 7. Block diagram of control circuitry.

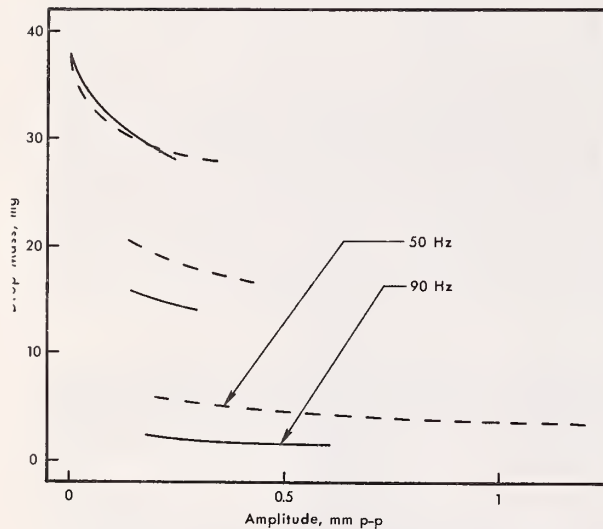


Figure 8. Variation of waterdrop mass with vibration amplitude at two fixed frequencies.

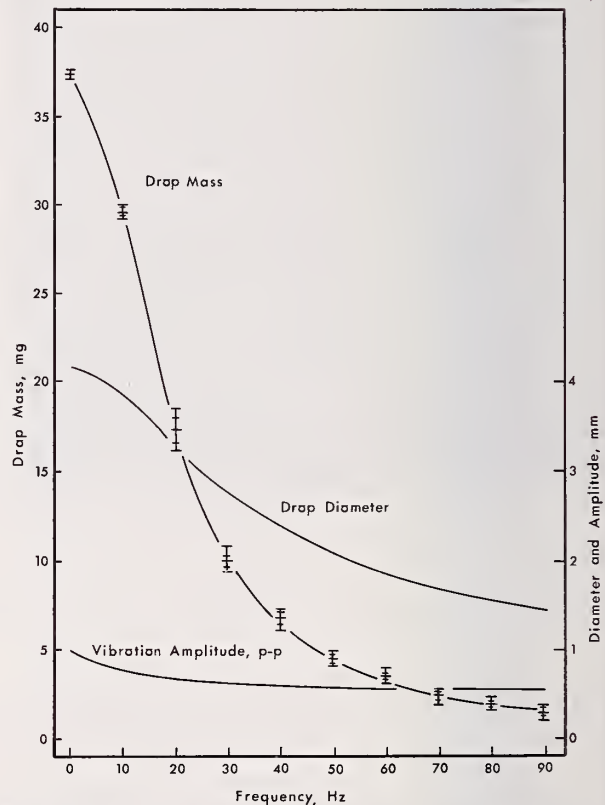


Figure 9. Waterdrop generator calibration data. Extreme bars at each date point represent extreme values of mass found at each frequency during calibration.

where the  $\sigma_i$  are the daily standard deviations at each frequency, and  $\sigma_w$  is the standard deviation of the weighing process, estimated to be 0.09 mg by weighing a 4.4 mg piece of wire several times and calculating the standard deviation. Note that on a percentage basis the standard deviations of the radii are one third the standard deviations of the masses reported in the table, since  $dm/m = 3 dr/r$  for a sphere; that is, the standard deviations of the radii range from .03 percent to 3.4 percent of the mean radii. The last two rows of the table show the drop diameters and the number of drops included in the data.

The calibration data are shown graphically in figure 9, where drop mass is plotted with respect to vibration frequency. The center bar at each data point represents the pooled average mass from table 1; the extreme bars represent the heaviest and lightest of all the drops generated at each frequency during calibration; and the other two bars represent the  $\sigma_{pc}$  from the table. Also shown in figure 9 are the vibration amplitude and the equivalent diameters for spherical drops.

To obtain further evidence of the resonant nature of the drop detachment process a small amount of water was admitted to the nozzle tip and then the flow stopped. The nozzle was then vibrated at the prescribed amplitude and the frequency swept toward the resonant frequency of the drop until the drop fell. Then the drop was weighed and the frequency recorded. The results are shown in table 2, where the calibration frequency is taken from figure 9 for the listed drop mass. Note that in most cases the drop fell slightly too soon (i.e., the nozzle frequency at detachment was too low when the frequency was swept upwards and too high when swept downwards). This probably indicates that the vibration amplitude was slightly higher than optimum. Some difficulty is encountered in the downward sweep, since the drop first must grow while the nozzle is still, then the nozzle vibration must grow slowly in amplitude without exciting higher modes of vibration of the hanging drop and causing it to fall.

In addition, observation under stroboscopic light confirms that the hanging waterdrop oscillates, with growing amplitude as the drop grows in mass, in the manner illustrated in figure 2. Furthermore, with the nozzle amplitude fixed below that required for detachment of the drop, the drop amplitude can be seen to grow, pass through a maximum, and then diminish as either the drop mass varies or the nozzle frequency varies sweeping the resonant frequency through the nozzle frequency or vice versa.

## 5. References

- [1] H. G. Wenzel, Jr. and R. Chun-Tsung Wang, "The Mechanics of a Drop After Striking a Stagnant Water Layer," Univ. of Ill. Water Resources Ctr. (1970).
- [2] G. L. Siscoe and Z. Levin, "Water Drop-Surface Wave Interactions," Univ. of Calif. at Los Angeles, Dept. of Meteorology (1971).
- [3] D. S. Chapman and P. R. Critchlow, J. Fluid Mech., 29, 1, 177 (1967).
- [4] D. C. Jenkins, Royal Aircraft Establishment, Tech. Rept. 66135 (1966).
- [5] D. P. Aeschliman, "An Experimental Study of the Response of Water Droplets to Flows Behind Plane Shock Waves," Sandia Labs. SC-RR-71 0540, (1971).
- [6] C. K. Mutchler, "Waterdrop Formation from Capillary Tubes," Agri. Res. Svc., ARS 41-107 (1965).
- [7] Lord Rayleigh, Proc. Roy. Soc., A 29, 71 (1879).
- [8] E. K. Dabora, Rev. Sci. Instr., 38, 502 (1967).
- [9] B. Raghupathy and S. B. Sample, Rev. Sci. Instr., 41, 645 (1970).
- [10] C. D. Hendricks and J. B. Y. Tsui, Rev. Sci. Instr., 39, 1088 (1968).
- [11] W. R. Atkinson and A. H. Miller, Rev. Sci. Instr., 36, 846 (1965).
- [12] B. J. Mason and J. L. Brownscombe, J. Sci. Instrum., 41, 258 (1964).
- [13] B. J. Mason, O. W. Jayaratne, J. D. Woods, J. Sci. Instrum., 40, 247 (1963).
- [14] R. H. Magarvey and B. W. Taylor, Rev. Sci. Instr., 27, 944 (1956).
- [15] K. Reil and J. Hallett, Rev. Sci. Instr., 40, 533 (1969).
- [16] W. R. Lane, J. Sci. Instrum., 24, 98 (1947).
- [17] P. V. Hobbs and A. J. Kezweeny, Science, 155, 1112 (1967).
- [18] J. E. Potzick, Rev. Sci. Instr., 39, 1219 (1968).
- [19] B. G. Kholin, Koklady, 15, 849 (1971).



Table 1. Waterdrop generator calibration data.

	Vibration Frequency, Hz									
	0	10	20	30	40	50	60	70	80	90
Day							Daily Average Mass, mg ( $\overline{m}_I$ )			
1	37.37	29.78	17.66	10.08	7.00	4.43	3.70	2.20	1.83	1.30
2	37.47	29.78	17.08	10.24	6.53	4.60	3.52	2.47	1.97	1.60
3	37.43	29.68	17.72	10.34	7.10	4.47	3.64	2.63	2.10	1.62
4	37.50	29.82	17.80	9.96	6.73	4.70	3.66	2.67	2.20	1.56
5	37.27	29.60	16.92	10.08	6.87	4.60	3.52	2.63	1.87	1.50
$\infty$										
$\overline{m}_p$	37.408	29.732	17.436	10.140	6.846	4.560	3.608	2.520	1.994	1.516
$\sigma_{pc}$	.033	.204	.710	.337	.383	.248	.141	.218	.118	.153
$\sigma_{pc}/\overline{m}_p$	0.09%	0.69	4.07	3.32	5.59	5.44	3.90	8.63	5.91	10.10
Drop Dia.	4.15 mm	3.84	3.22	2.69	2.30	2.06	1.90	1.69	1.56	1.43
No. of Drops	15	25	25	25	15	15	25	15	15	25

Table 2. Drop detachment with swept nozzle frequency.

<u>Drop Mass</u>	<u>Nozzle Frequency</u>	<u>Calibration Frequency</u>	<u>Sweep Direction</u>
11.1 mg	27.8 Hz	28.5 Hz	Up
10.6	28.1	29.0	Up
5.7	42.8	44.0	Up
16.0	22.4	21.3	Up
18.0	23.4	19.3	Down
24.6	19.1	14.2	Down
17.6	21.6	19.7	Down

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. NBS TN-776	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE  A NEW METHOD FOR GENERATING WATERDROPS OF SPECIFIED MASS		5. Publication Date May 1973	
		6. Performing Organization Code	
7. AUTHOR(S) James E. Potzick		8. Performing Organization	
9. PERFORMING ORGANIZATION NAME AND ADDRESS  NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		10. Project/Task/Work Unit No. 2130470	
		11. Contract/Grant No. NAonr 4-72	
12. Sponsoring Organization Name and Address  Fluid Dynamics Program Office of Naval Research Department of the Navy Arlington, Virginia 22217		13. Type of Report & Period Covered Final	
		14. Sponsoring Agency Code	
15. SUPPLEMENTARY NOTES			
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.)  A waterdrop generator has been constructed, based on the mechanical resonance of a vibrating waterdrop, which can generate drops of 1.5 to 37 mg with standard deviations in the range of 0.1 percent to 10 percent of drop mass. Drop mass over this range and drop interval are remotely controlled.			
17. KEY WORDS (Alphabetical order, separated by semicolons)  Drop generator; liquid drop; waterdrop			
18. AVAILABILITY STATEMENT  <input checked="" type="checkbox"/> UNLIMITED.  <input type="checkbox"/> FOR OFFICIAL DISTRIBUTION. DO NOT RELEASE TO NTIS.		19. SECURITY CLASS (THIS REPORT)  UNCLASSIFIED	21. NO. OF PAGES  12
		20. SECURITY CLASS (THIS PAGE)  UNCLASSIFIED	22. Price \$.35 Domestic postpaid \$.25 G.P.O. Bookstore



## PERIODICALS

**JOURNAL OF RESEARCH** reports National Bureau of Standards research and development in physics, mathematics, and chemistry. Comprehensive scientific papers give complete details of the work, including laboratory data, experimental procedures, and theoretical and mathematical analyses. Illustrated with photographs, drawings, and charts. Includes listings of other NBS papers as issued.

*Published in two sections, available separately:*

• **Physics and Chemistry (Section A)**

Papers of interest primarily to scientists working in these fields. This section covers a broad range of physical and chemical research, with major emphasis on standards of physical measurement, fundamental constants, and properties of matter. Issued six times a year. Annual subscription: Domestic, \$17.00; Foreign, \$21.25.

• **Mathematical Sciences (Section B)**

Studies and compilations designed mainly for the mathematician and theoretical physicist. Topics in mathematical statistics, theory of experiment design, numerical analysis, theoretical physics and chemistry, logical design and programming of computers and computer systems. Short numerical tables. Issued quarterly. Annual subscription: Domestic, \$9.00; Foreign, \$11.25.

## TECHNICAL NEWS BULLETIN

The best single source of information concerning the Bureau's measurement, research, developmental, cooperative, and publication activities, this monthly publication is designed for the industry-oriented individual whose daily work involves intimate contact with science and technology—for engineers, chemists, physicists, research managers, product-development managers, and company executives. Includes listing of all NBS papers as issued. Annual subscription: Domestic, \$6.50; Foreign, \$8.25.

## NONPERIODICALS

**Applied Mathematics Series.** Mathematical tables, manuals, and studies.

**Building Science Series.** Research results, test methods, and performance criteria of building materials, components, systems, and structures.

**Handbooks.** Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

**Special Publications.** Proceedings of NBS conferences, bibliographies, annual reports, wall charts, pamphlets, etc.

**Monographs.** Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

**National Standard Reference Data Series.** NSRDS provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated.

**Product Standards.** Provide requirements for sizes, types, quality, and methods for testing various industrial products. These standards are developed cooperatively with interested Government and industry groups and provide the basis for common understanding of product characteristics for both buyers and sellers. Their use is voluntary.

**Technical Notes.** This series consists of communications and reports (covering both other-agency and NBS-sponsored work) of limited or transitory interest.

**Federal Information Processing Standards Publications.** This series is the official publication within the Federal Government for information on standards adopted and promulgated under the Public Law 89-306, and Bureau of the Budget Circular A-86 entitled, Standardization of Data Elements and Codes in Data Systems.

**Consumer Information Series.** Practical information, based on NBS research and experience, covering areas of interest to the consumer. Easily understandable language and illustrations provide useful background knowledge for shopping in today's technological marketplace.

## BIBLIOGRAPHIC SUBSCRIPTION SERVICES

The following current-awareness and literature-survey bibliographies are issued periodically by the Bureau:

**Cryogenic Data Center Current Awareness Service** (Publications and Reports of Interest in Cryogenics).

A literature survey issued weekly. Annual subscription: Domestic, \$20.00; foreign, \$25.00.

**Liquefied Natural Gas.** A literature survey issued quarterly. Annual subscription: \$20.00.

**Superconducting Devices and Materials.** A literature survey issued quarterly. Annual subscription: \$20.00.

Send subscription orders and remittances for the preceding bibliographic services to the U.S. Department of Commerce, National Technical Information Service, Springfield, Va. 22151.

**Electromagnetic Metrology Current Awareness Service** (Abstracts of Selected Articles on Measurement Techniques and Standards of Electromagnetic Quantities from D-C to Millimeter-Wave Frequencies). Issued monthly. Annual subscription: \$100.00 (Special rates for multi-subscriptions). Send subscription order and remittance to the Electromagnetic Metrology Information Center, Electromagnetics Division, National Bureau of Standards, Boulder, Colo. 80302.

Order NBS publications (except Bibliographic Subscription Services) from: Superintendent of Documents, Government Printing Office, Washington, D.C. 20402.

**U.S. DEPARTMENT OF COMMERCE**  
**National Bureau of Standards**  
Washington, D.C. 20234

OFFICIAL BUSINESS

Penalty for Private Use, \$300

POSTAGE AND FEES PAID  
U.S. DEPARTMENT OF COMMERCE  
COM-215

